
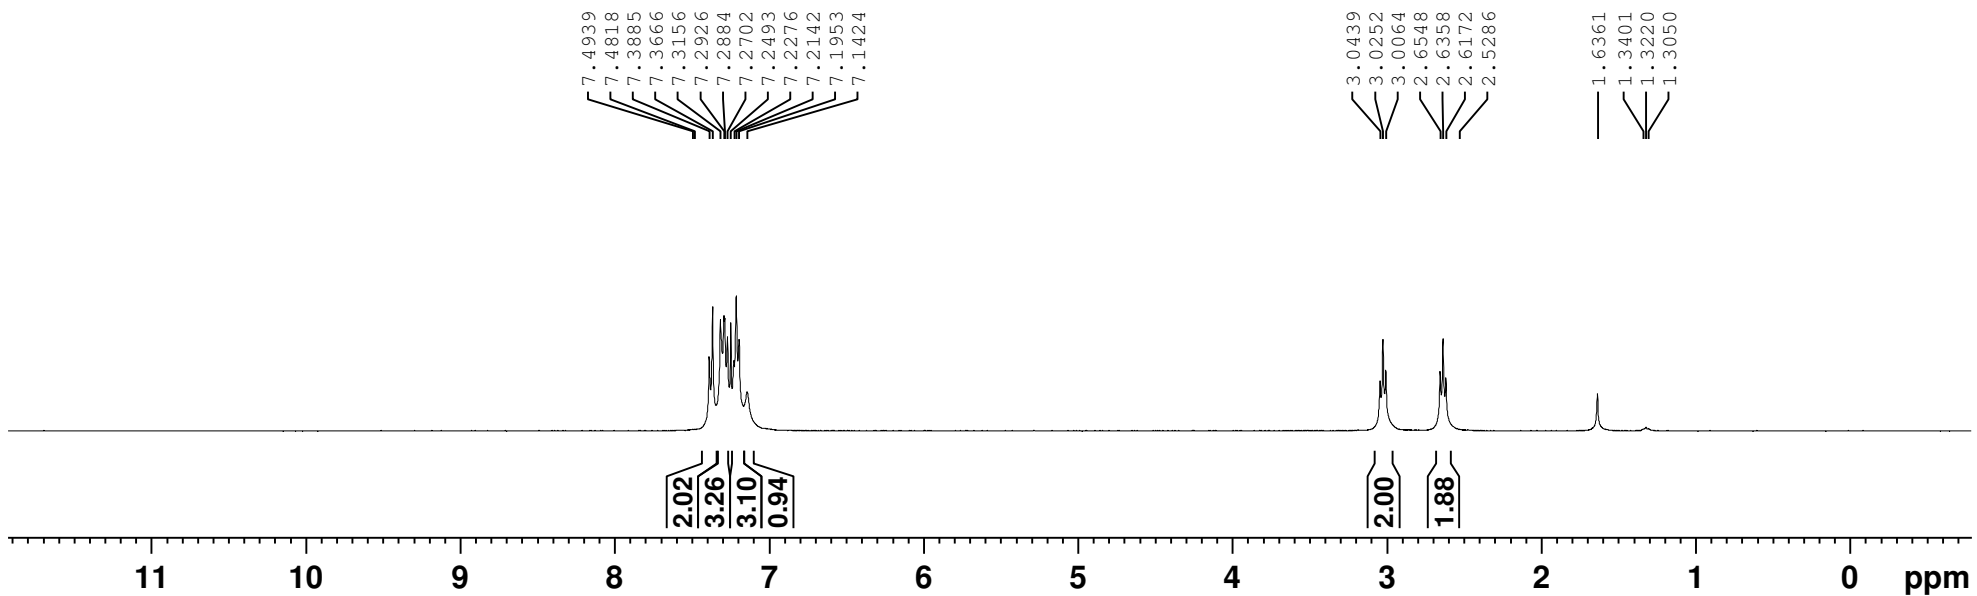


Kolkata

Current Data Parameters  
 NAME CR592-17852-74-P  
 EXPNO 10  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20220520  
 Time 16.58 h  
 INSTRUM spect  
 FREQHD Z8246\_0048 (PH)  
 PULPROG zg30  
 TD 24036  
 SOLVENT CDCl3  
 NS 8  
 DS 0  
 SWH 8012.820 Hz  
 FIDRES 0.666735 Hz  
 AQ 1.4998465 sec  
 RG 203  
 DW 62.400 usec  
 DE 6.50 usec  
 TE 300.0 K  
 D1 1.00000000 sec  
 TD0 1  
 SFO1 400.1024006 MHz  
 NUC1 1H  
 P1 18.00 usec  
 PLW1 10.00000000 W


F2 - Processing parameters  
 SI 16384  
 SF 400.1000139 MHz  
 WDW EM  
 SSB 0  
 LB 0 Hz  
 GB 0  
 PC 1.00

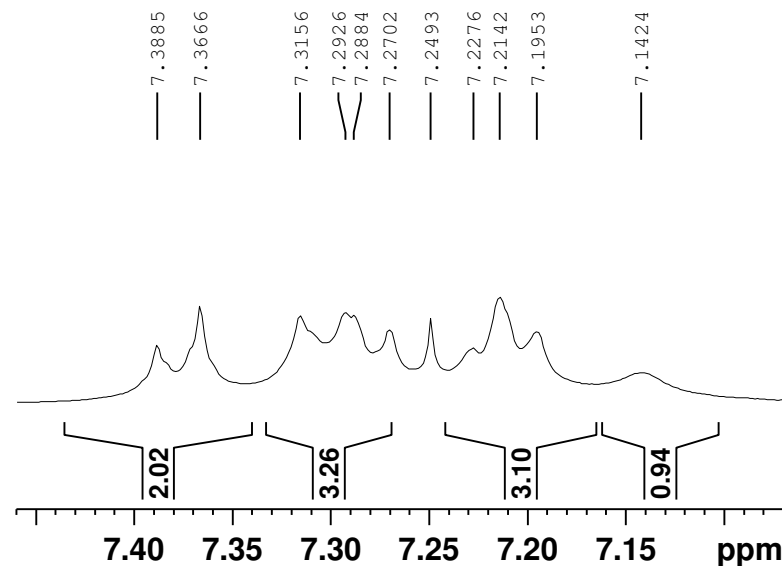

Author: Erhard Mettler  
 Date: 20-05-2022  
 Database: STARe Default DB V15.00: METTLER

TCG LIFESCIENCES PVT LTD

**Evaluation:**

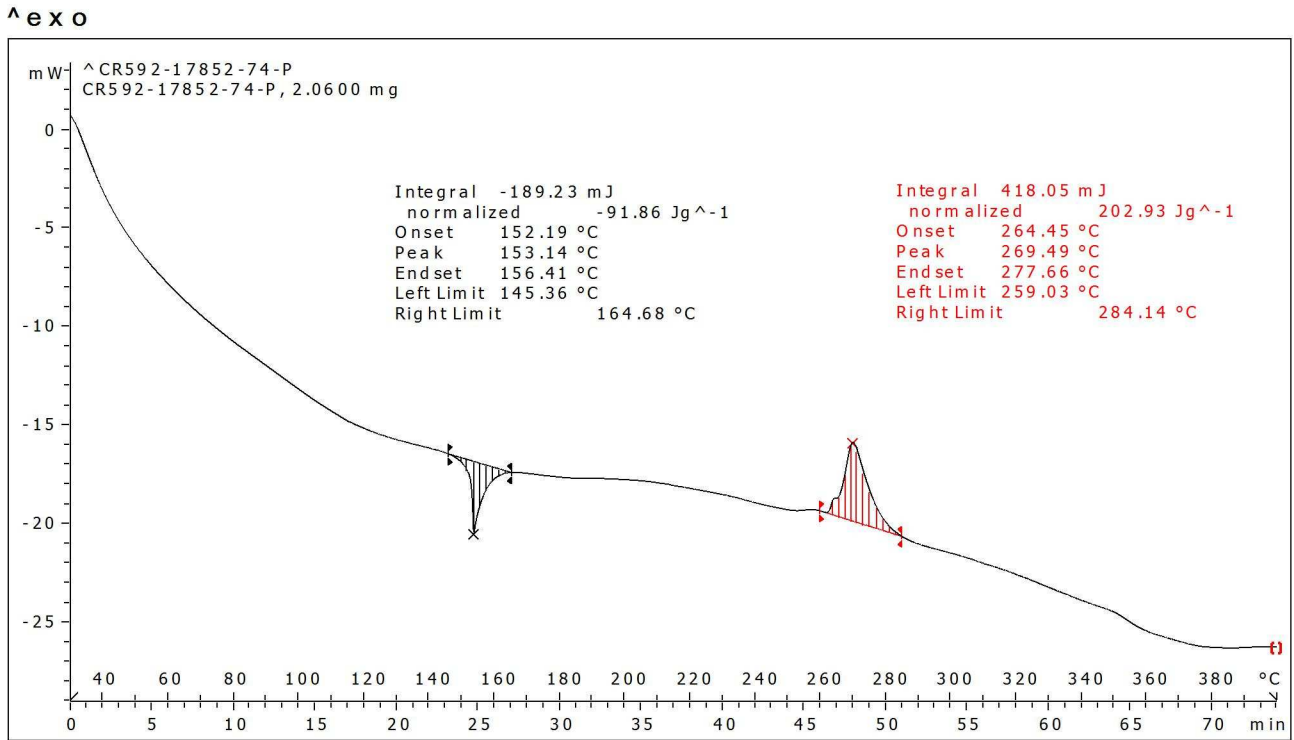

TCG Lifesciences Pvt Ltd: METTLER


STAR<sup>e</sup> SW 15.00

**Curve:** CR592-17852-74-P, 20.05.2022 18:04:47  
**Sample:** CR592-17852-74-P, 2.0600 mg  
**Sample Holder:** HP Gold Plated 40ul  
 Weight : 0  
 Material: Stainless Steel  
**Method:** 30-400@5°C/MIN, N2 40.0 ML/MIN-Gold  
 dt 1.00 s  
 [1] 30.0..400.0 °C, 5.00 K/min, N2 40.0 ml/min  
 Synchronization enabled  
**Module:** DSC 3 /500/887, 05.05.2017 15:16:17  
**User:** METTLER


SAMPLE INFORMATION

Sample Name:	CR592-17852-74-P	Acquired By:	ah0113531
Sample Type:	Unknown	Sample Set Name:	BDQ_CP_210522_01
Vial:	66	Acq. Method Set:	BDQ_CP_LC42_01
Injection #:	1	Processing Method:	BDQ_CP_230522_01
Injection Volume:	10.00 ul	Channel Name:	240.0nm
Run Time:	40.0 Minutes	Proc. Chnl. Descr.:	2998 PDA 240.0 nm (2998)
Date Acquired:	21-05-2022 18:22:12 IST	Column Name:	SIMPAK SOLAR C-18(250X4.6)mm,5μ
Date Processed:	23-05-2022 08:14:09 IST		

Auto-Scaled Chromatogram

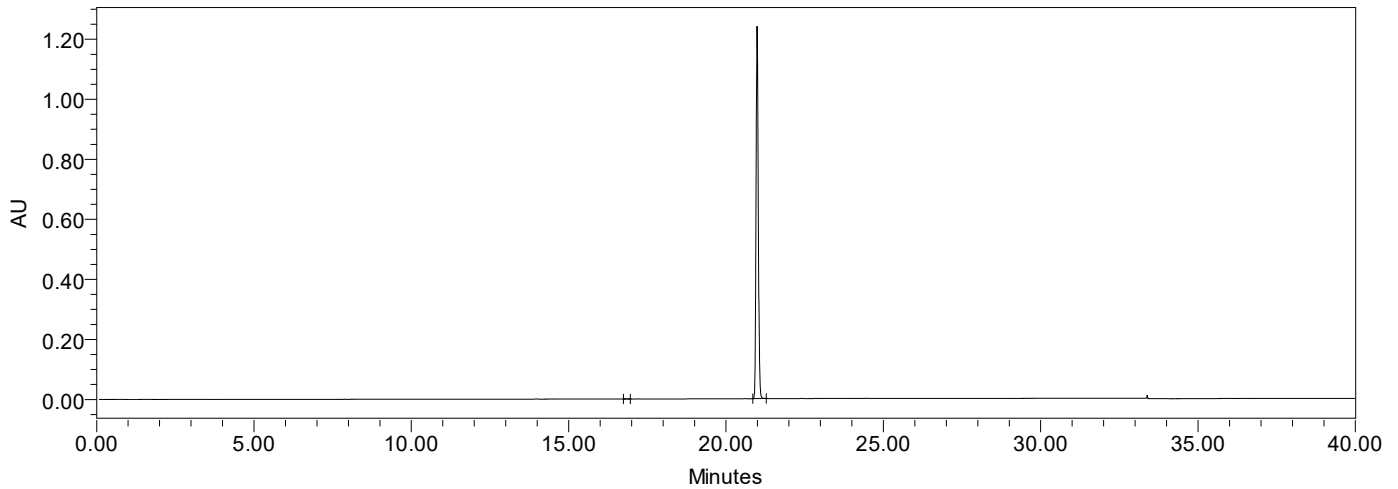

Zoom- Chromatogram

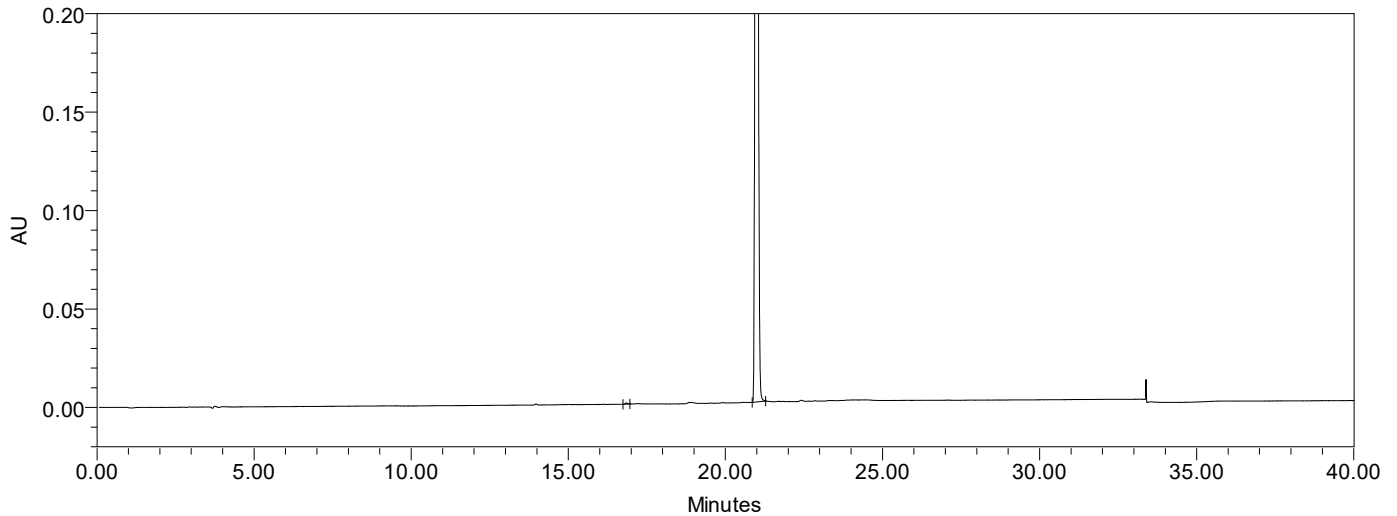


### Peak Results

	Name	RT	Area	% Area	RT Ratio
1	Peak2	16.847	3236	0.05	0.80
2	COMP-2	20.988	6027592	99.95	1.00


SAMPLE INFORMATION

Sample Name:	CR592-17852-74-RM	Acquired By:	SS0113466
Sample Type:	Unknown	Sample Set Name:	BDQ_CP_200522_01
Vial:	10	Acq. Method Set:	BDQ_CP_LC42_01
Injection #:	1	Processing Method:	BDQ_CP_200522_01
Injection Volume:	10.00 ul	Channel Name:	240.0nm
Run Time:	40.0 Minutes	Proc. Chnl. Descr.:	2998 PDA 240.0 nm (2998)
Date Acquired:	20-05-2022 08:12:55 IST	Column Name:	SIMPAK SOLAR C-18(250X4.6)mm,5μ
Date Processed:	20-05-2022 09:06:56 IST		

Auto-Scaled Chromatogram

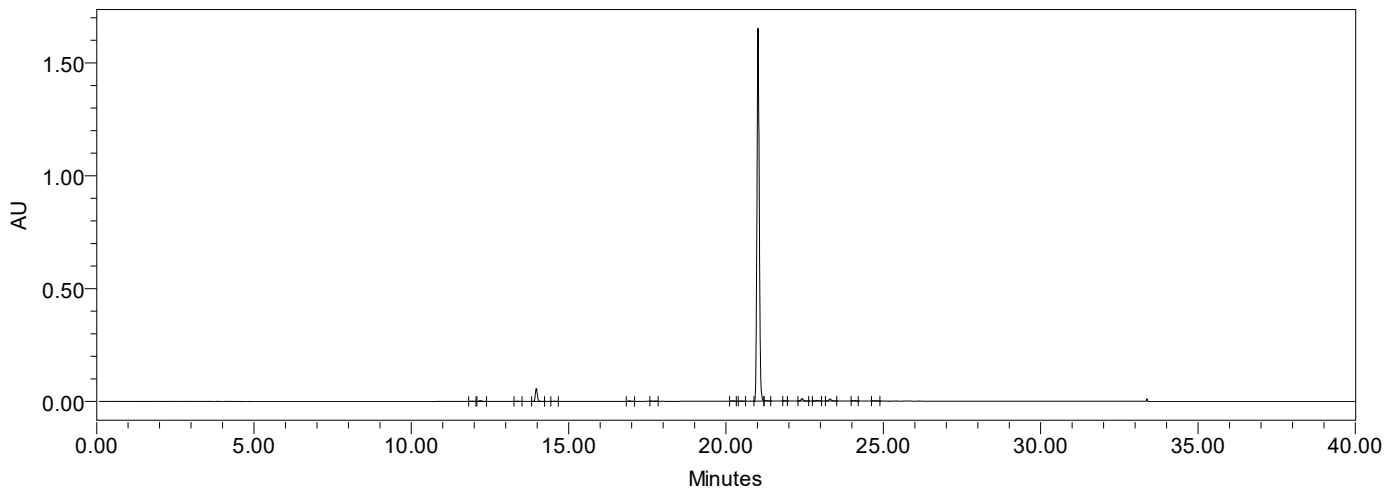

Zoom- Chromatogram

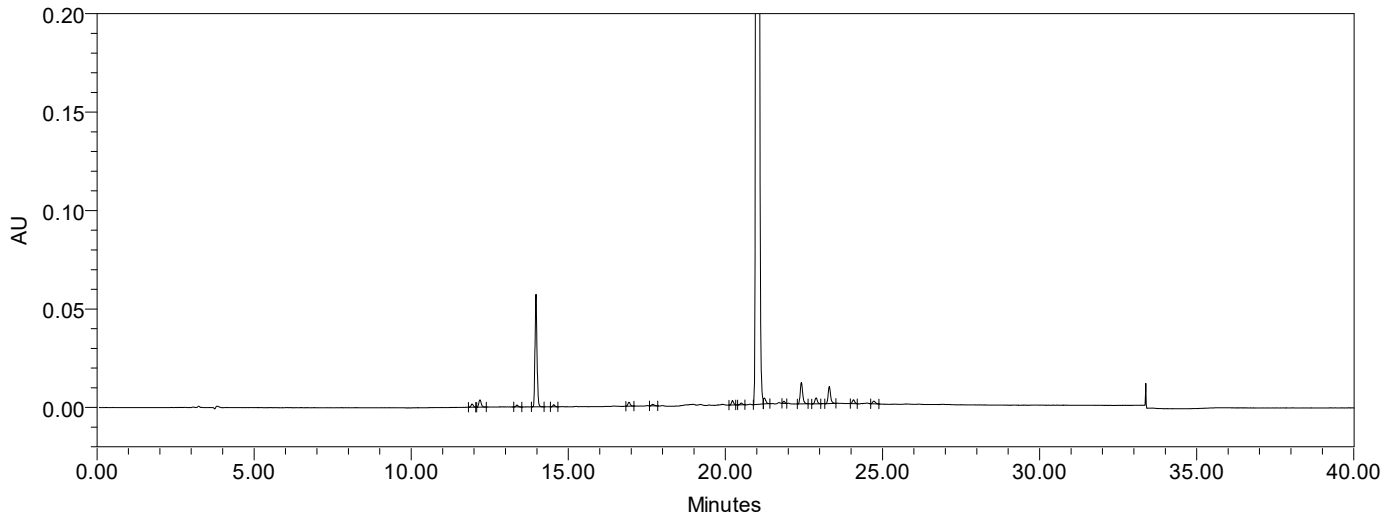

### Peak Results

	Name	RT	Area	% Area	RT Ratio
1	Peak1	11.937	7690	0.09	0.57
2	Peak2	12.188	19723	0.23	0.58
3	Peak3	13.364	4212	0.05	0.64
4	Peak4	13.970	249828	2.85	0.66
5	Peak5	14.537	5034	0.06	0.69
6	Peak6	16.932	9856	0.11	0.81
7	Peak7	17.684	4633	0.05	0.84
8	Peak8	20.225	10392	0.12	0.96
9	Peak9	20.502	4465	0.05	0.98
10	COMP	21.017	8283809	94.59	1.00
11	Peak11	21.244	15173	0.17	1.01
12	Peak12	21.863	4432	0.05	1.04
13	Peak13	22.415	58027	0.66	1.07
14	Peak14	22.885	15880	0.18	1.09
15	Peak15	23.306	45934	0.52	1.11
16	Peak16	24.075	10165	0.12	1.15
17	Peak17	24.725	8520	0.10	1.18